


# Andover Corporation

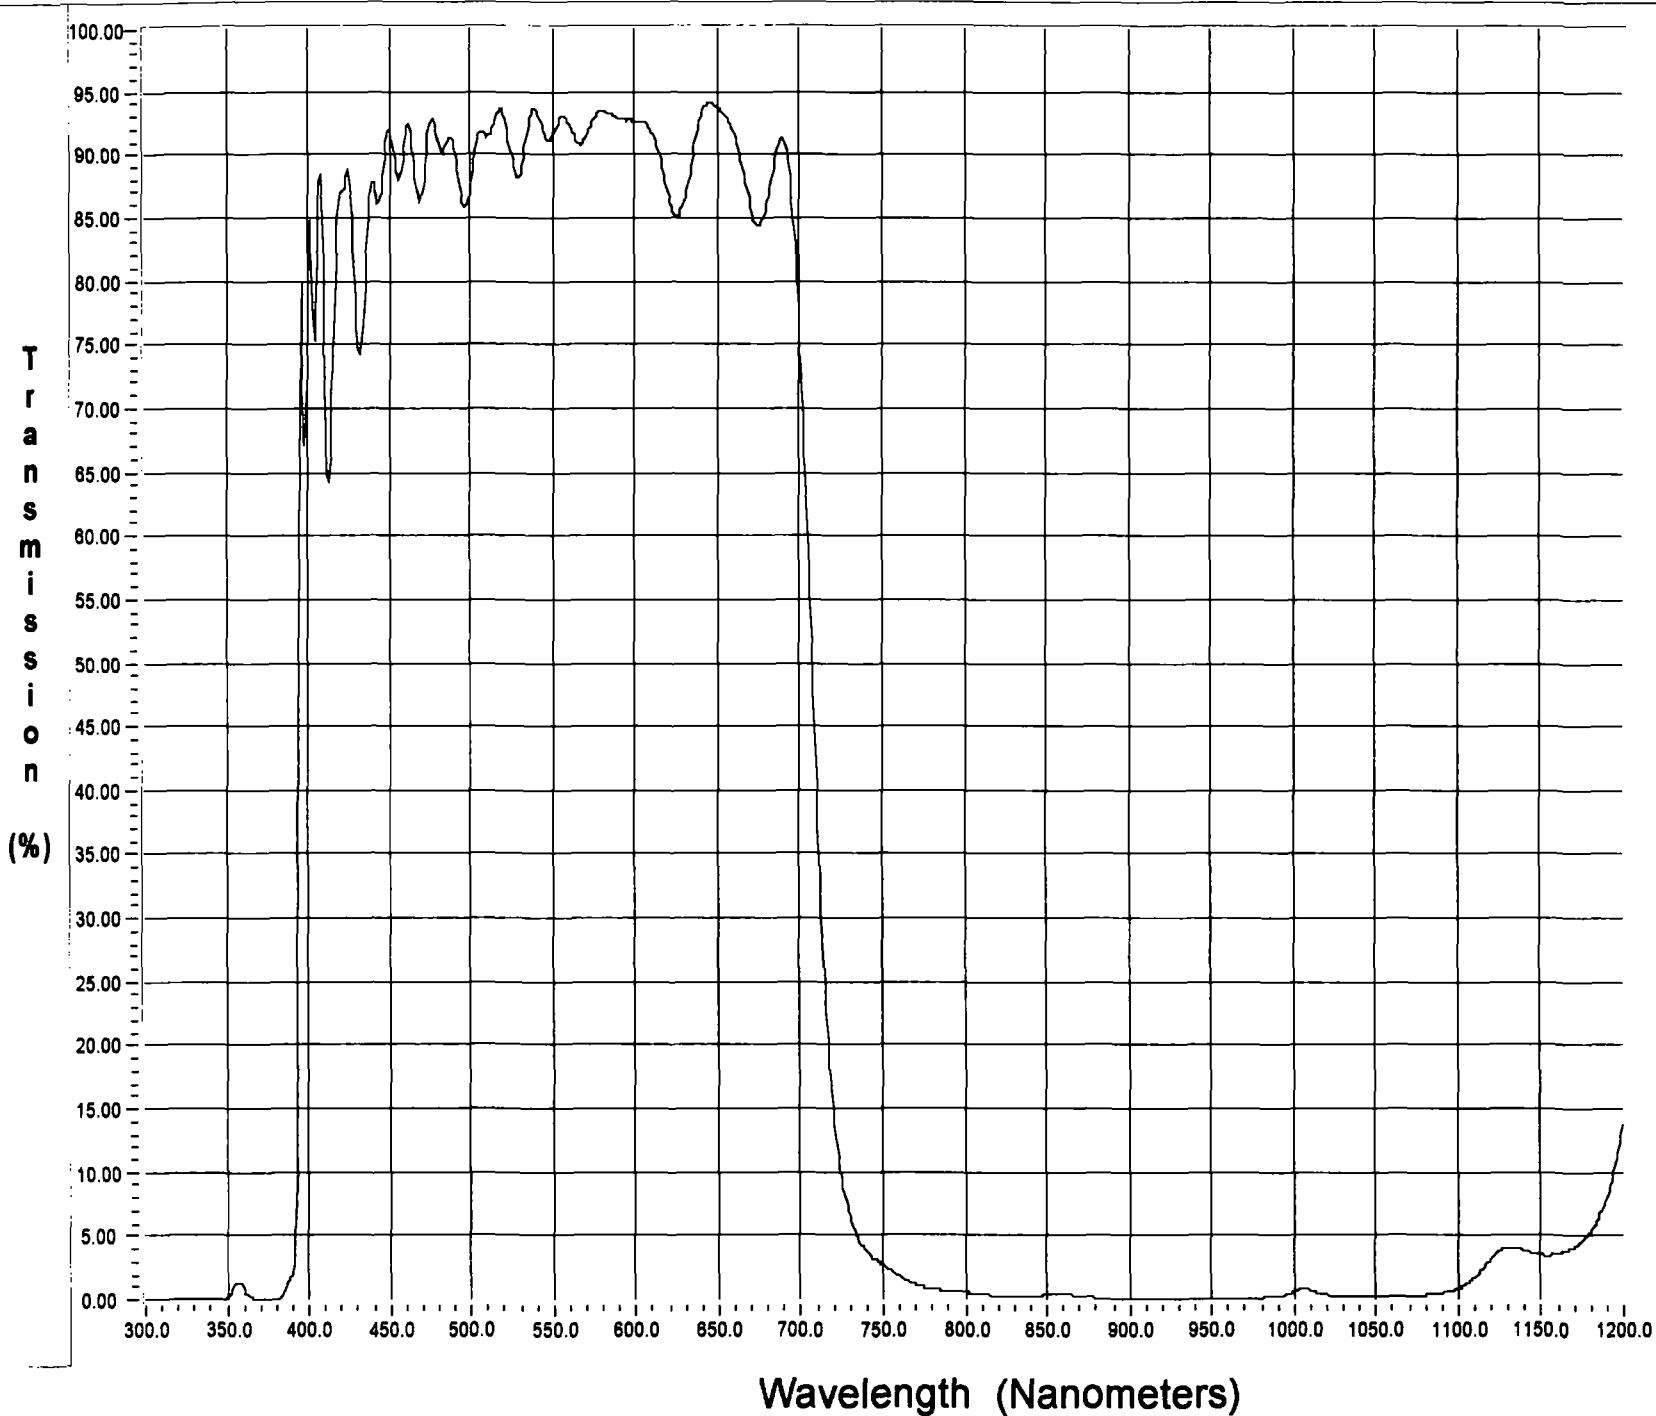

## Filter I.D.

Test Instrument:

Cary 500 (1437)

Test Technician:

J. Moreau *jme*

Date:

Fri, Aug 29, 2003

Customer Name:

University of California

Job Number:

AM-53808

Part Number:

ANDV8970

Serial Number:

01

Lot Number:

21161

## Filter Data

Transmission average from:

450nm - 675nm: 90.852%

750nm - 1200nm: 1.234%

Polarization:

RANDOM

Angle of Incidence:

0.00°

Ambient Temperature:

23.0° C.

# Andover Corporation

4 Commercial Drive, Salem, NH 03079 USA  
Telephone: (603) 893-6888 Fax: (603) 893-6508

Web site: [www.andcorp.com](http://www.andcorp.com)  
e-mail: [crichards@andcorp.com](mailto:crichards@andcorp.com)



Christopher A. Richards  
Quality Control Manager

Optical components for research and industry