

# Nikon

## Stereoscopic Microscope

# SMZ-2B

### INSTRUCTIONS

#### CAUTIONS

**1. Avoid sharp knocks!**

When carrying the microscope, or manipulating, handle the microscope gently taking care to avoid sharp knocks.

**2. Locations of microscope**

Avoid the following conditions: dust, vibration and exposure to high temperature, moisture or direct sunlight.

**3. Dirt on the lens**

Do not leave dust, dirt or finger marks on the lens surfaces. They will prevent you from clear observation of the specimen image.

absolute alcohol (ethyl alcohol or methyl alcohol) be used.

Observe sufficient caution in handling alcohol.

**2. Cleaning the plastic parts**

Avoid the use of any organic solvent (for example, thinner, ether, alcohol, xylene etc.) for cleaning the plastic parts and painted surfaces of the instrument.

**3. Never attempt to dismantle!**

Never attempt to dismantle the instrument so as to avoid the possibility of impairing the operational efficiency and accuracy.

**4. When not in use**

When not in use, cover the instrument with the accessory vinyl cover, and store it in a place free from moisture and fungus.

#### MAINTENANCE

**1. Cleaning the lenses**

To clean the lens surfaces, remove dust using soft brush or gauze. Only for removing finger marks or grease, should soft cotton cloth, lens tissue or gauze lightly moistened with

**5. Periodical checking**

To maintain the performance of the instrument, we recommend to check the instrument periodically. (For details for this check, contact your dealer.)

NIKON CORPORATION

---

## NOMENCLATURE AND USING

### Eyepieces

The eyepieces available as standard for the Microscope SMZ-2B are 10X and 15X. 20X and 33X are also available on order.

Note that no regular (biological) microscope eyepiece can be used interchangeably.

### Diopter rings

Provided on both the righthand and lefthand eyepieces and adjustable to prevent out-of-focus during the time of zooming.

### Microscope body

### Microscope body clamp screw

For fastening firmly the main body of Microscope SMZ-2B onto the focus stand.

### Episcopic illuminator

Incorporates a halogen lamp 6V-10W, illumination angle is changeable. To achieve the most appropriate illumination for observation, adjust the position of the lamp.

### Clips

To hold the specimen in place securely.

### Stage plate

The black or opal surface is to be used according to the specimen to be observed. On the diasopic illuminator base, use the transparent glass plate.

### Zooming knob


Rotation of the zooming knob changes the magnifying power of the objective continuously from 0.8X to 5X, the powers being indicated on the knob.

### Flexible arm attaching screws

Provided on both the right and left sides of the focus stand arm and used to attach the flexible arm.

### Focus knobs

Rotation of the knobs moves the main body of microscope. For increasing the tightness of rotation turn the right-and lefthand knobs in the opposite directions, i.e. in the fastening direction for each knob, as indicated by the arrow "TENSION" marked on the knobs. The tightness will be decreased by releasing the each knob at the same time.

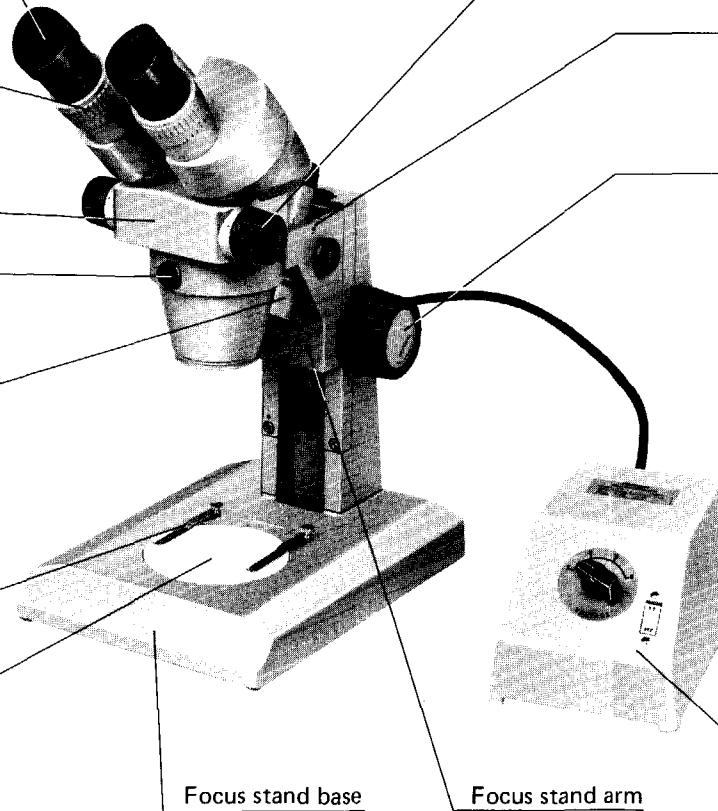

## OPERATING PROCEDURE

1. Place the specimen onto the stage plate.
2. Turn both diopter rings on the binocular tubes until the 0 line to the index.
3. Looking into the eyepieces of the binocular tubes, adjust the interpupillary distance by moving the binocular tubes, so that both the circular viewfields are brought into coincidence.
4. Set the zooming knob to 5X.
5. Rotating the focus knobs, bring the specimen image into focus. If, beforehand, the distance between the specimen and the bottom of the microscope main body is made about 100mm, focusing will be facilitated.
6. Rotate the zooming knob to 0.8X.
7. Manipulating the right- and lefthand diopter rings one after the other, bring the images into focus independently.
8. Repeat the above procedures from 4. to 7. to make sure of exact focusing, and, then the image will keep its sharpness all the time of continuous magnification changes by zooming.

## MAGNIFICATION TABLE

Objective	Auxiliary objectives	Working distance (mm)	Eyepieces							
			10X Field number 23		15X Field number 14		20X Field number 12		33X Field number 5	
			Total magnification	Real field (mm)	Total magnification	Real field (mm)	Total magnification	Real field (mm)	Total magnification	Real field (mm)
0.8~5X	—	100	8~50X	28.8~4.6	12~75X	17.5~2.8	16~100X	15~2.4	26.4~165X	6.3~1
	0.5X	181	4~25X	57.6~9.2	6~37.5X	35.0~5.6	8~50X	30~4.8	13.2~82.5X	12.6~2
	2X	32.7	16~100X	14.4~2.3	24~150X	8.75~1.4	32~200X	7.5~1.2	52.8~330X	3.1~0.5

*We reserve the right to make such alterations in design as we may consider necessary in the light of experience. For this reason, particulars and illustrations in this handbook may not conform in every detail to models in current production.*

## ACCESSORIES

<b>Eyepieces:</b>	20× and 33×
<b>Auxiliary objectives:</b>	0.27×, 0.4×, 0.5×, 0.7×, 1.5× and 2.0× (with 0.5× objective, use Extension ring)
<b>Universal illuminator</b>	
<b>Fluorescent ring illuminator</b>	
<b>Fiber optics illuminators:</b>	Bifurcated and Ring illuminators
<b>Diascopic illuminator base</b>	
<b>Episcopic illuminator:</b>	Incorporates a halogen lamp 6V—10W (G.E. No. 787)
<b>Flexible supporting arm</b>	
<b>Universal arm</b>	
<b>Universal stand:</b>	Table stand and Table clamp stand

## NIKON CORPORATION

9-16, Ohi 3-chome, Shinagawa-ku, Tokyo 140, Japan  
Tel: +81-3-3773-8122 Fax: +81-3-3773-8115

## NIKON INC.

### Instrument Group

1300 Walt Whitman Road, Melville, NY 11747-3064, U.S.A.  
Tel: +1-516-547-8500 Fax: +1-516-547-0306

## NIKON EUROPE B.V.

Schipholweg 321, P.O. Box 222, 1170 AE Badhoevedorp, The Netherlands  
Tel: +31-20-44-96-222 Fax: +31-20-44-96-299

## NIKON AG

Kaspar-Fennerstrasse 6, 8700 Küsnacht, Zürich, Schweiz  
Tel: +41-1-913-62-00 Fax: +41-1-910-37-44

## NIKON GMBH

Tiefenbroicher Weg 25 40472 Düsseldorf 30, Fed. Rep. of Germany  
Tel: +49-0211-94-14-0 Fax: +49-0211-94-14-322

## NIKON FRANCE S.A.

191, rue du Marche Rollay, 94504 Champigny Sur Marne Cedex France  
Tel: +33-1-45 16 45 16 Fax: +33-1-45 16 00 33

## NIKON INSTRUMENTS S.P.A.

Via Tevere, 54 50019 Sesto Fiorentino (Fl), Italia  
Tel: +39-55-3009601 Fax: +39-55-300993

## NIKON U.K. LTD.

380 Richmond Road, Kingston, Surrey KT2 5PR, United Kingdom  
Tel: +44-181-541-4440 Fax: +44-181-541-4564



Printed in Japan

66 E 91.6.E.13