

# Instructions

**Tektronix**

**P2100 100 MHz  
1X/10X Passive Probe  
071-0774-01**



071077401

Copyright © Tektronix, Inc. All rights reserved.

Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supercedes that in all previously published material. Specifications and price change privileges reserved.

Tektronix, Inc., P.O. Box 500, Beaverton, OR 97077

TEKTRONIX and TEK are registered trademarks of Tektronix, Inc.

## WARRANTY

Tektronix warrants that the products that it manufactures and sells will be free from defects in materials and workmanship for a period of one (1) year from the date of shipment. If a product proves defective during this warranty period, Tektronix, at its option, either will repair the defective product without charge for parts and labor, or will provide a replacement in exchange for the defective product.

In order to obtain service under this warranty, Customer must notify Tektronix of the defect before the expiration of the warranty period and make suitable arrangements for the performance of service. Customer shall be responsible for packaging and shipping the defective product to the service center designated by Tektronix, with shipping charges prepaid. Tektronix shall pay for the return of the product to Customer if the shipment is to a location within the country in which the Tektronix service center is located. Customer shall be responsible for paying all shipping charges, duties, taxes, and any other charges for products returned to any other locations.

This warranty shall not apply to any defect, failure or damage caused by improper use or improper or inadequate maintenance and care. Tektronix shall not be obligated to furnish service under this warranty a) to repair damage resulting from attempts by personnel other than Tektronix representatives to install, repair or service the product; b) to repair damage resulting from improper use or connection to incompatible equipment; c) to repair any damage or malfunction caused by the use of non-Tektronix supplies; or d) to service a product that has been modified or integrated with other products when the effect of such modification or integration increases the time or difficulty of servicing the product.

**THIS WARRANTY IS GIVEN BY TEKTRONIX IN LIEU OF ANY OTHER WARRANTIES, EXPRESS OR IMPLIED. TEKTRONIX AND ITS VENDORS DISCLAIM ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. TEKTRONIX' RESPONSIBILITY TO REPAIR OR REPLACE DEFECTIVE PRODUCTS IS THE SOLE AND EXCLUSIVE REMEDY PROVIDED TO THE CUSTOMER FOR BREACH OF THIS WARRANTY. TEKTRONIX AND ITS VENDORS WILL NOT BE LIABLE FOR ANY INDIRECT, SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES IRRESPECTIVE OF WHETHER TEKTRONIX OR THE VENDOR HAS ADVANCE NOTICE OF THE POSSIBILITY OF SUCH DAMAGES.**

# Contacting Tektronix

Product support	<p>For questions about using Tektronix measurement products, call toll free in North America: 1-800-833-9200 6:00 a.m. – 5:00 p.m. Pacific time</p> <p>Or contact us by e-mail: tm_app_supp@tek.com</p> <p>For product support outside of North America, contact your local Tektronix distributor or sales office.</p>
Service support	<p>Tektronix offers a range of services, including Extended Warranty Repair and Calibration services. Contact your local Tektronix distributor or sales office for details.</p> <p>For a listing of worldwide service centers, visit our web site.</p>
Toll-free Number	<p>In North America: 1-800-833-9200 An operator can direct your call.</p>
Postal Address	<p>Tektronix, Inc. Department or name (if known) P.O. Box 500 Beaverton, OR 97077 USA</p>
Web site	<p><a href="http://www.tektronix.com">www.tektronix.com</a></p>

# General Safety Summary

Review the following safety precautions to avoid injury and prevent damage to this product or any products connected to it. To avoid potential hazards, use this product only as specified.

*Only qualified personnel should perform service procedures.*

## To Avoid Fire or Personal Injury

**Connect and Disconnect Properly.** Do not connect or disconnect probes or test leads while they are connected to a voltage source.

**Connect and Disconnect Properly.** Connect the probe output to the measurement instrument before connecting the probe to the circuit under test. Disconnect the probe input and the probe ground from the circuit under test before disconnecting the probe from the measurement instrument.

**Observe All Terminal Ratings.** To avoid fire or shock hazard, observe all ratings and markings on the product. Consult the product manual for further ratings information before making connections to the product.

Connect the ground lead of the probe to earth ground only.

**Do Not Operate Without Covers.** Do not operate this product with covers or panels removed.

**Avoid Exposed Circuitry.** Do not touch exposed connections and components when power is present.

**Do Not Operate With Suspected Failures.** If you suspect there is damage to this product, have it inspected by qualified service personnel.

**Do Not Operate in Wet/Damp Conditions.**

**Do Not Operate in an Explosive Atmosphere.**

**Keep Product Surfaces Clean and Dry.**

## Safety Terms and Symbols

**Terms in This Manual.** These terms may appear in this manual:



---

**WARNING.** *Warning statements identify conditions or practices that could result in injury or loss of life.*

---



---

**CAUTION.** *Caution statements identify conditions or practices that could result in damage to this product or other property.*

---

**Terms on the Product.** These terms may appear on the product:

**DANGER** indicates an injury hazard immediately accessible as you read the marking.

**WARNING** indicates an injury hazard not immediately accessible as you read the marking.

**CAUTION** indicates a hazard to property including the product.

**Symbols on the Product.** These symbols may appear on the product:



CAUTION  
Refer to Manual



Double  
Insulated



Protective Ground  
(Earth) Terminal





# P2100 Passive Probe

The P2100 is a compact, 1.5 meter passive probe with selectable 1X/10X attenuation. The probe is designed for use with general purpose oscilloscopes with input capacitance between 18 and 35 pF. There are no user-serviceable parts in the P2100 probe.




## Features and Accessories

Table 3 shows the features and accessories of the P2100 probe.

**Table 3: Features and standard accessories**

Feature/Accessory	Description
	<p><b>Probe attenuation.</b> This switch selects the attenuation factor of the probe.</p>
 <p style="text-align: center;">Hook tip</p>	<p><b>Hook tip.</b> Connects the probe tip to wires and component leads for hands-free measurement.</p> <p><i><b>NOTE.</b> For a solid connection, firmly push and twist the hook tip onto the probe tip before using.</i></p> <p>Replacement part number: 013-0318-00</p>
 <p style="text-align: center;">Color marker bands</p>	<p><b>Color marker bands.</b> Attach matching pairs of the color marker bands onto the strain-relief sections of cable at the probe head and compensation box. When several probes are connected to an instrument, the color marker bands enable quick verification of which probe is connected to which instrument channel.</p> <p>Replacement part number: 016-0633-00</p>
	<p><b>Ground lead.</b> Use the ground lead for connecting the probe ground to the circuit.</p> <p>Replacement part number: 196-3466-00</p>

**Table 3: Features and standard accessories (Cont.)**

Feature/Accessory	Description
 An adjustment tool with a long handle and a cylindrical body with a BNC connector at the end. The handle has a textured grip.	<p><b>Adjustment tool.</b> Used to adjust probe compensation. Access the adjustment through the opening near the BNC connector.</p> <p>Replacement part number: 003-1873-00</p>
 A small, rectangular manual or booklet.	<p><b>Instructions.</b> Provides instructions for operating the probe.</p> <p>Replacement part number: 071-0774-01</p>
 A finger guard, which is a ring-shaped component that fits around the probe tip. An arrow points to it with the label "Finger guard".	<p><b>Guard.</b> Keeps fingers away from the probe tip for protection against electric shock.</p>



---

**WARNING.** To avoid electric shock when using the probe, keep fingers behind the guard on the probe body.

---



## Probe Compensation

Due to variations in oscilloscope input characteristics, probe low-frequency compensation may need adjustment after moving the probe from one oscilloscope to another. If a 1 kHz calibrated square wave displayed at 1 ms/division shows significant differences between the leading and trailing edges, perform the following steps to optimize low-frequency compensation.

2. Connect the probe to the calibration signal on the oscilloscope front panel.
3. Press **AUTOSET** or otherwise adjust your digitizing oscilloscope to display a meaningful waveform.
4. Adjust the trimmer in the probe until you see a perfectly flat-top square wave on the display. See Figure 4.

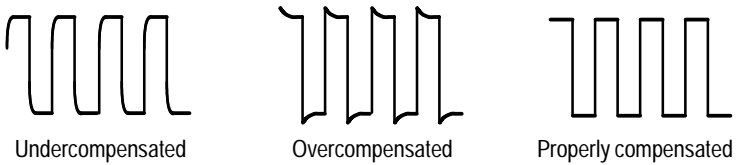



Figure 4: Probe compensation waveforms

## Specifications

**Table 4: Electrical characteristics**

	10X position	1X position
Bandwidth	DC to 100 MHz	DC to 7 MHz
Attenuation ratio	10:1	1:1
Compensation Range	18 pF-35 pF	All oscilloscopes with 1 M $\Omega$ input
Input resistance	10 M $\Omega \pm 2\%$	1 M $\Omega \pm 2\%$
Input capacitance	14.5 pF-17.5 pF	80 pF-110 pF
Maximum input voltage <sup>1</sup>	10X position	300 V RMS CAT I or 300 V DC CAT I 300 V RMS CAT II or 300 V DC CAT II 100 V RMS CAT III or 100 V DC CAT III 420 V peak, <50% DF, <1 sec PW 670 V peak, <20% DF, <1 sec PW
	1X position	150 V RMS CAT I or 150 V DC CAT I 150 V RMS CAT II or 150 V DC CAT II 100 V RMS CAT III or 100 V DC CAT III 210 V peak, <50% DF, <1 sec PW 330 V peak, <20% DF, <1 sec PW

**1** As defined in EN61010-1. See Certifications and compliances in Table 5.

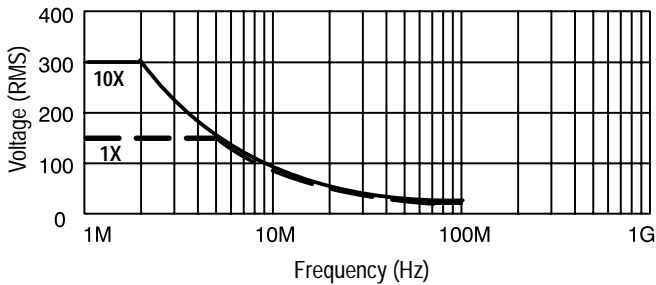

**Figure 5: Derating curve for determining maximum input voltage**

**Table 5: Certifications and compliances**

EC Declaration of Conformity	<p>Compliance was demonstrated to the following specification as listed in the Official Journal of the European Communities:</p> <p>Low Voltage Directive 73/23/EEC as amended by 93/68/EEC:</p> <p>EN 61010-1/A2 Safety requirements for electrical equipment for measurement, control, and laboratory use</p> <p>EN61010-2-031: Particular requirements for hand-held probe assemblies for electrical measurement and test 1994</p>
Overvoltage Category	<p>Category:            Examples of Products in this Category:</p> <p>CAT III                Distribution-level mains, fixed installation</p> <p>CAT II                 Local-level mains, appliances, portable equipment</p> <p>CAT I                  Signal levels in special equipment or parts of equipment, telecommunications, electronics</p>
Pollution Degree 2	Do not operate in environments where conductive pollutants may be present.
Safety	<p>UL3111-1, First Edition &amp; IEC61010-2-031, First Edition          CSA C22.2 No. 1010.1-92 &amp; CAN/CSA C22.2 No. 1010.2.031-94          EN61010-1/A2          EN61010-2-031          Pollution Degree 2</p>

**Table 6: Environmental characteristics**

Temperature	Operating	0° C to +50° C
	Nonoperating	-20° C to +60° C
Cooling Method	Convection	
Humidity	+40° C or below	≤ 90% relative humidity
	+41° C to +50° C	≤ 60% relative humidity
Altitude	Operating	3,000 m
	Nonoperating	15,000 m