

MICRO



GILMONT
INSTRUMENTS, INC.


Calibration Chart

Flowmeter Catalog No. F3000

Serial No. 804

$D_1 = 0.394"$ $W_1 = .00209$ GM $\rho_1 = 3.98$ GM/ML

** MEASURED AND FLOWING AT 1 ATM. AND 70° F.

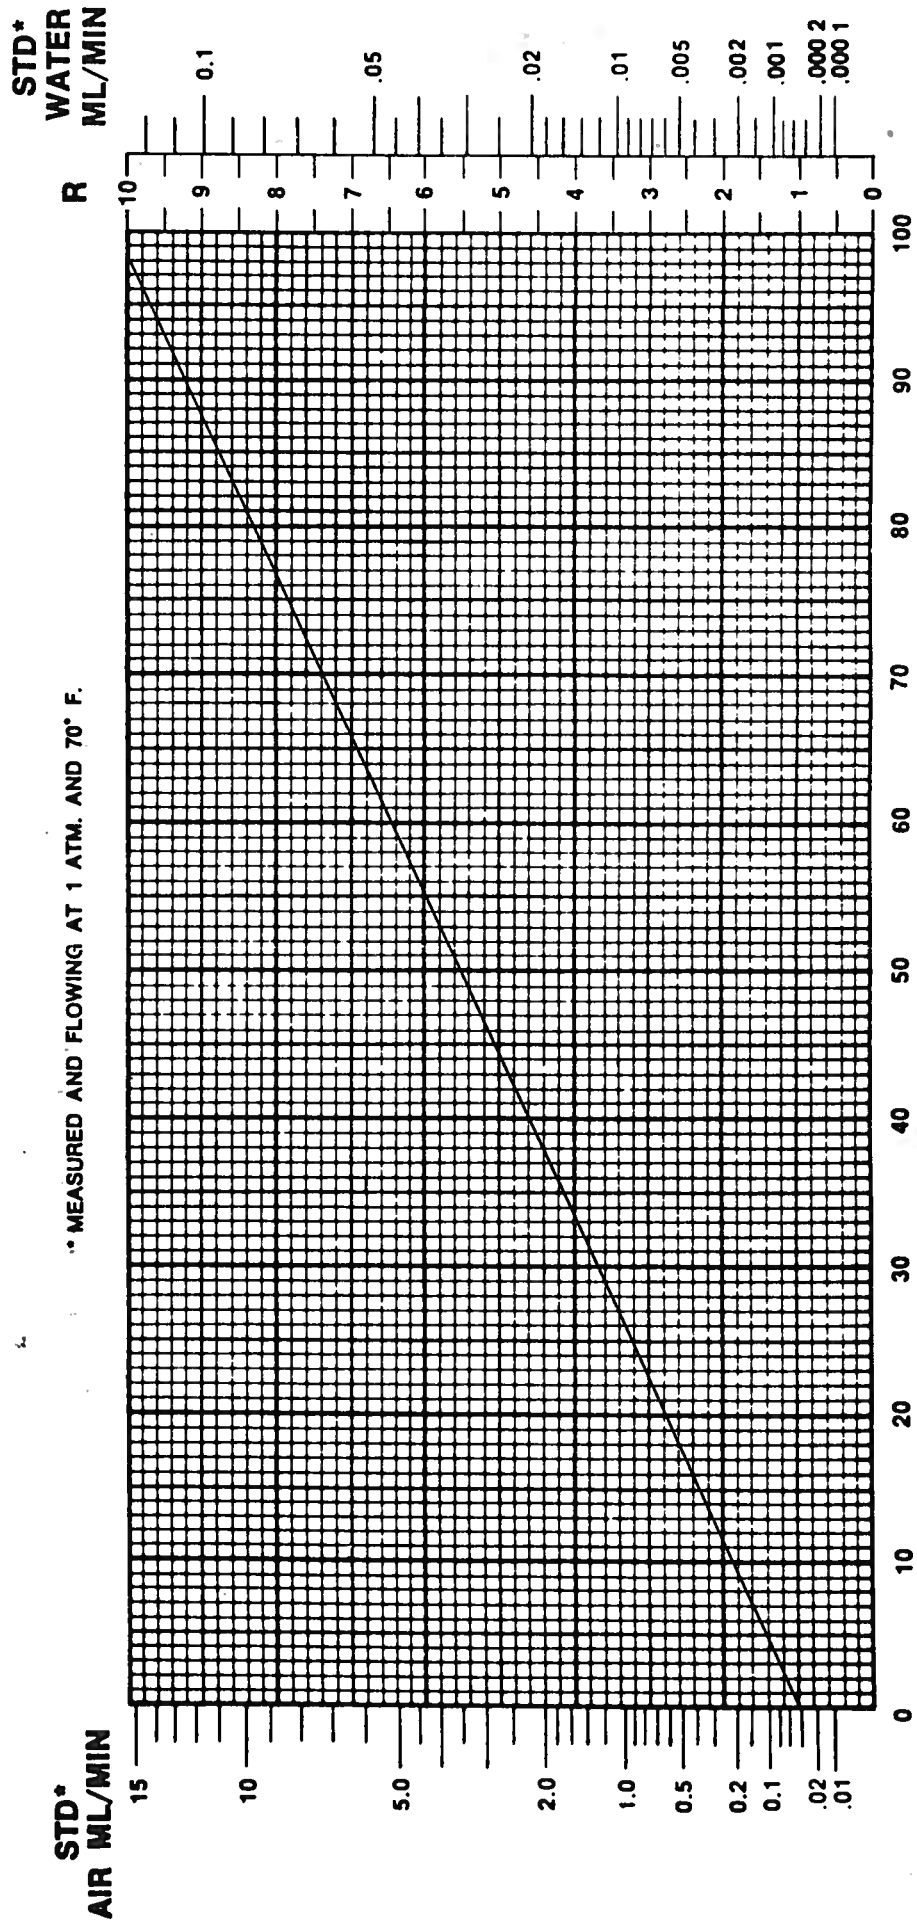

SCALE READING AT CENTER OF BALL